



pH MODULE

FOR SOIL MACRONUTRIENTS KIT · CODE 5928-01

OCTA-SLIDE 2, pH 4.0 - 9.0

CODE 5935-01

QUANTITY	CONTENTS	CODE
15 mL	*Tricon pH Indicator	*5937-E
120 mL	Tricon Flocculating Reagent	5941PS-J
120 mL	Tricon Flocculating Reagent	5941PT-J
2	Test Tubes, w/caps	0845
1	Spoon, 0.5g, plastic	0698
1	pH Soil Octa-Slide 2 Bar, 4.0-9.0	5936-01
1	Octa-Slide 2 Viewer	1101

***WARNING:** Reagents marked with an * are considered to be potential health hazards. To view or print a Safety Data Sheet (SDS) for these reagents go to www.lamotte.com. Search for the four digit reagent code number listed on the reagent label, in the contents list or in the test procedures. Omit any letter that follows or precedes the four digit code number. For example, if the code is 4450WT-H, search 4450. To obtain a printed copy, contact LaMotte by email, phone or fax.


Emergency information for all LaMotte reagents is available from Chem-Tel: (US, 1-800-255-3924) (International, call collect, 813-248-0585).

To order individual reagents or test kit components, use the specified code number.

For the interpretation of the pH test and a discussion of its importance, see *A Study of Soil Science* (Code 1530) by Dr. Henry D. Foth.





Warning! This set contains chemicals that may be harmful if misused. Read cautions on individual containers carefully. Not to be used by children except under adult supervision.

USE OF THE OCTA-SLIDE 2 VIEWER



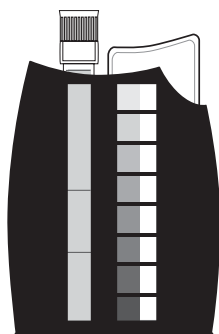


The Octa-Slide 2 Viewer should be held so non-direct light enters through the back of the Viewer. Insert the Octa-Slide 2 Bar into the Viewer. Insert the reacted sample into the top of the Viewer. Match the color of the reaction to the color standards.

PROCEDURE

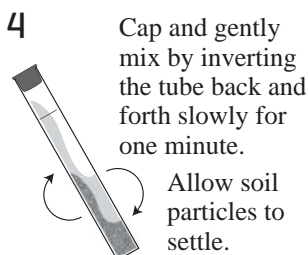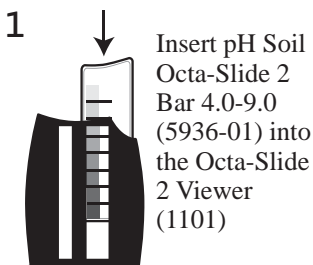

NOTE: The amount of time required for a soil to settle varies with texture; clay soils may require additional time, but in most instances the solution will be clear in several minutes.

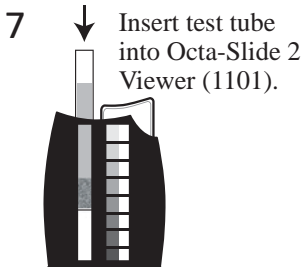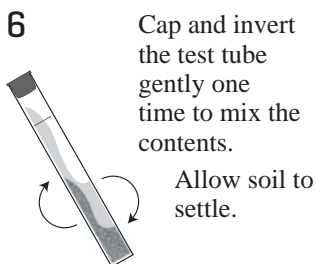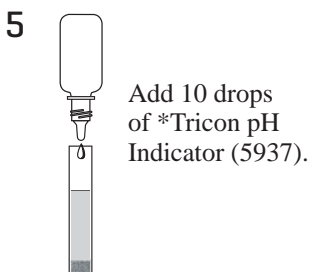

LaMOTTE COMPANY

Helping People Solve Analytical Challenges

PO Box 329 · Chestertown · Maryland · 21620 · USA
800-344-3100 · 410-778-3100 [Outside U.S.A.] · Fax: 410-778-6394

Visit us on the web at www.lamotte.com